

## Wireless Tracking System for Disabled People Using GSM Technology

**Boda Sairam**

**M.Tech(Embedded Systems & VLSI Design),  
Malla Reddy Institute of Technology and Science.**

**K.V.Phani Raja, M.Tech**

**Assistant Professor,  
Malla Reddy Institute of Technology and Science.**


### Introduction:

The patient monitoring systems is one of the major improvements in the hospitality because of its advanced technology. This project is designed for convenience of patient using embedded technology. In this project simultaneously monitor the patient's condition. It is to operate and available at an affordable cost.

### Existing method:

This project describes the design of a simple, low-cost controller based wireless Patient monitoring system. A panic switch is also interfaced to the controller that is to send a signal by the patient if anything is wrong or else if the patient needs some attention then they can press the switch. The signal through the panic switch is sent the remote place using GSM module interfaced to the controller.

### Block Diagram

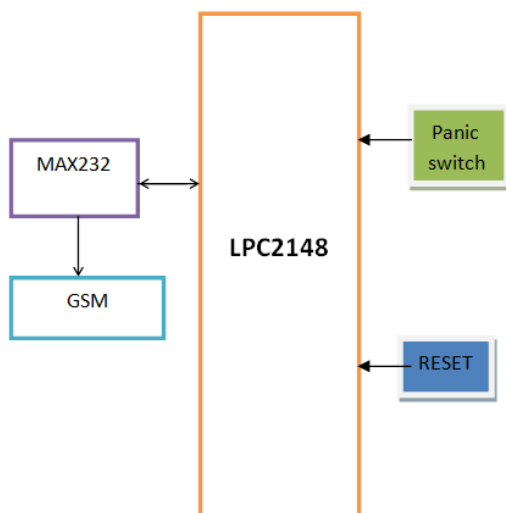


### Draw backs

Here the patient himself need to know about his condition and react and he need to press the switch. This may not be possible all the time and the patient may fall in danger. There were no sensors used to monitor his condition which is a major drawback and we can overcome this by using sensors to measure heart rate and temperature.

### Proposed method:


This project describes the design of a simple, low-cost controller based wireless Patient monitoring system. Heart rate of the patient is measured from the thumb finger using IRD (Infra Red Device sensors).A panic switch is also interfaced to the controller that is to send a signal by the patient if anything is wrong or else if the patient needs some attention then they can press the switch. Heart rate values and the signal through the panic switch is sent the remote place using GSM module interfaced to the controller. A GPS module is also interfaced to get the location value of the patient.

Block Diagram

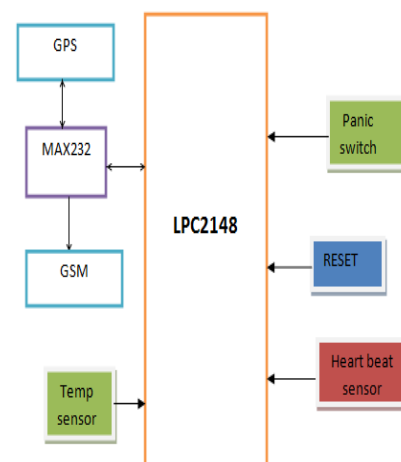

## Modules used in this project

The **LPC2148** are based on a 16/32 bit ARM7TDMI-S™ CPU with real-time emulation and embedded trace support, together with 128/512 kilobytes of embedded high speed flash memory. A 128-bit wide memory interface and unique accelerator architecture enable 32-bit code execution at maximum clock rate. For critical code size applications, the alternative 16-bit Thumb Mode reduces code by more than 30% with minimal performance penalty. With their compact 64 pin package, low power consumption, various 32-bit timers, 4- channel 10-bit ADC, USB PORT, PWM channels and 46 GPIO lines with up to 9 external interrupt pins these microcontrollers are particularly suitable for industrial control, medical systems, access control and point-of-sale. With a wide range of serial communications interfaces, they are also very well suited for communication gateways, protocol converters and embedded soft modems as well as many other general-purpose applications.

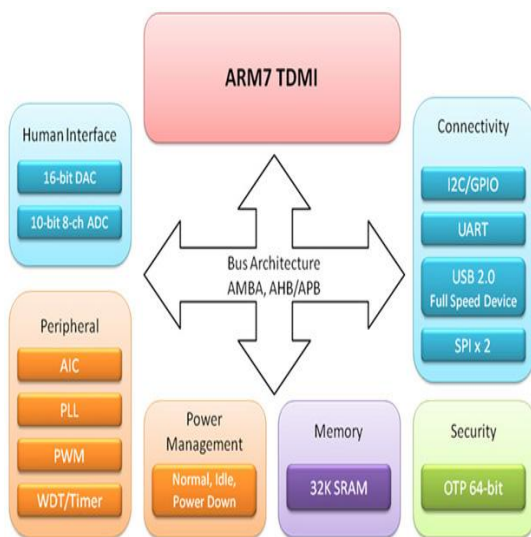

This project uses regulated 3.3V, 500mA power supply. Unregulated 12V DC is used for relay. 7805 three terminal voltage regulator is used for voltage regulation. Bridge type full wave rectifier is used to rectify the ac output of secondary of 230/12V step down transformer.

## ARM7TDMI Processor Core

- Current low-end ARM core for applications like digital mobile phones
- TDMI
  - T: Thumb, 16-bit compressed instruction set
  - D: on-chip Debug support, enabling the processor to halt in response to a debug request
  - M: enhanced Multiplier, yield a full 64-bit result, high performance
  - I: Embedded ICE hardware
- Von Neumann architecture

## Global System for Mobile Communication (GSM)

### Definition:

GSM, which stands for Global System for Mobile communications, reigns (important) as the world's most widely used cell phone technology. Cell phones use a cell phone service carrier's GSM network by searching for cell phone towers in the nearby area. Global system for mobile communication (GSM) is a globally accepted standard for digital cellular communication. GSM is the name of a standardization group established in 1982 to create a common European mobile telephone standard that would formulate specifications for a pan-European mobile cellular radio system operating at 900 MHz. It is estimated that many countries outside of Europe will join the GSM partnership.

### MODEM SPECIFICATIONS:


The SIM300 is a complete Tri-band GSM solution in a compact plug-in module. Featuring an industry-standard interface, the SIM300 delivers GSM/GPRS900/1800/1900Mhz performance for voice, SMS, data and Fax in a small form factor and

with low power consumption. The leading features of SIM300 make it deal with virtually unlimited application, such as WLL applications (Fixed Cellular Terminal), M2M application, handheld devices and much more.

1. Tri-band GSM/GPRS module with a size of 40x33x2.85
2. Customized MMI and keypad/LCD support
3. An embedded powerful TCP/IP protocol stack
4. Based upon mature and field proven platform, backed up by our support service, from definition to design and production.

### General Features:

- Tri-band GSM/GPRS900/1800/1900MHz
- GPRS multi-slot class 10
- GPRS mobile station class –B
- Complaint to GSM phase 2/2+
  - i. -class 4(2W @900MHz)
  - ii. -class 1(1W @/18001900MHz)
- Dimensions: 40x33x2.85 mm
- Weight: 8gm
- Control via AT commands
- (GSM 07.07, 07.05 and SIMCOM enhanced AT commands)
- SIM application tool kit
- supply voltage range 3.5.....4.5 v
- Low power consumption
- Normal operation temperature: -20 °C to +55 °C
- Restricted operation temperature : -20 °C to -25 °C and +55 °C to +70 °C
- storage temperature: -40 °C to +80 °C

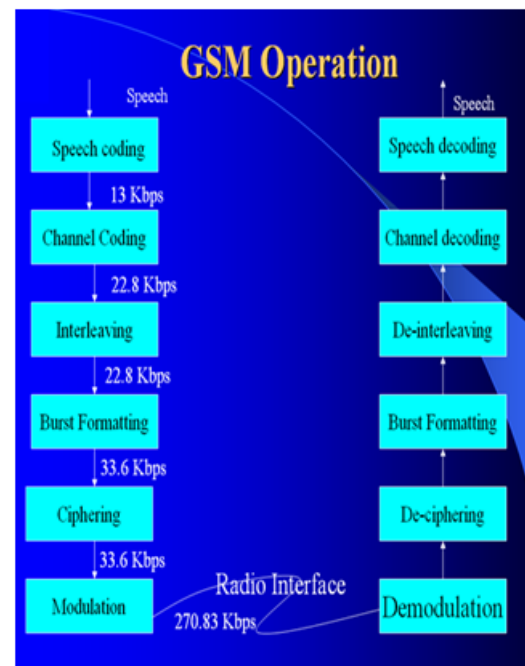

### Global Positioning System:

The Global Positioning System (GPS) is a U.S. space-based global navigation satellite system. It provides reliable positioning, navigation, and timing services to worldwide users on a continuous basis in all weather, day and night, anywhere on or near the Earth which has an unobstructed view of four or more GPS satellites. GPS is made up of three segments: Space, Control and User. The Space Segment is composed of 24 to 32 satellites in Medium Earth Orbit and also includes the boosters required to launch them into orbit. The Control Segment is composed of a Master Control Station, an Alternate Master Control Station, and a host of dedicated and shared Ground Antennas and Monitor Stations. The User Segment is composed of hundreds of thousands of U.S. and allied military users of the secure GPS Precise Positioning Service, and tens of millions of civil, commercial and scientific users of the Standard Positioning Service (see GPS navigation devices). GPS satellites broadcast signals from space that GPS receivers use to provide three-dimensional location (latitude, longitude, and altitude) plus precise time.

**Blood Pressure Meter:**

A sphygmomanometer (blood pressure meter, or blood pressure gauge (also referred to as a sphygmometer) is a device used to measure blood pressure, composed of an inflatable cuff to restrict blood flow, and a mercury or mechanical manometer to measure the pressure. It is always used in conjunction with a means to determine at what pressure blood flow is just starting, and at what pressure it is unimpeded. Manual sphygmomanometers are used in conjunction with a stethoscope. The word comes from the Greek (*sphygmos*, pulse), plus the scientific term manometer (pressure meter). The device was invented by Samuel Siegfried Karl Ritter von Basch in 1881. Scipione Riva-Rocci introduced a more easily used version in 1896. In 1901, Harvey Cushing modernized the device and popularized it within the medical community. A sphygmomanometer consists of an inflatable cuff, a measuring unit (the mercury manometer, or aneroid gauge), and a mechanism for inflation which may be a manually operated bulb and valve or a pump operated electrically. The usual unit of measurement of blood pressure is millimeters of mercury (mmHg) as measured directly by a manual sphygmomanometer.



**Pulse counting sensor:**

Heart rate is the speed of people's emotional state, exercise intensity and objective indicator of cardiac function. But most people are very difficult to accurately measure the time and his heart rate values. If the heart rate monitor with me, heart ECG electrodes

will be detected by monitoring the signal processing device, the user can at any time that your heart rate changes, changes in heart rate, self-monitoring status.



Heart rate monitor for heart rate range (60 ~ 160) / min. Circuit by adjusting the relevant components, in the (60 ~ 160) / min within the audible alarm can change the heart rate range. This heart rate range the width of the design center values  $\pm 20\%$  range. If central values such as emphasis on the 100 / exceptionally, the heart rate signal range (80 ~ 120) / min, if the heart rate exceeds this range, the lower limit, the instrument does not sound, if the heart rate in the range of the instrument ECG is the sound issue.

**LM35**

**FEATURES DESCRIPTION**

- Calibrated Directly in ° Celsius (Centigrade)
- Linear + 10 mV/°C Scale Factor • 0.5°C Ensured Accuracy (at +25°C) • Rated for Full -55°C to +150°C Range
- Suitable for Remote Applications
- Low Cost Due to Wafer-Level Trimming
- Operates from 4 to 30 V
- Less than 60-μA Current Drain
- Low Self-Heating, 0.08°C in Still Air





[8]Kenneth.J.Ayala,"The 8051 Microcontroller Architecture programming and Applications", 2nd Edition.

[9]Janicegillispie Mazidi, Muhammad Ali Mazidi,"The 8051Microcontroller and Embedded System", 2nd Edition, Person Education 2009.

[10]Webster John G.," Medical Instrumentation. Application and Design", 3rd Edition Wiley, 1998.

[11]Ramakant A. Gayakwad, "Op-amps and linear integrated circuits", 2<sup>nd</sup> Edition Prentice Hall, 2000..

[12]ECG Measurement System -Chia-Hung Chen, Shi-Gun Pan, Peter Kinget.

[13]Daniel Paulus / Thomas Meier,"ECG-Amplifier", MB Jass 2009.

[14]G.M.Patil, K.Subbarao, V.D.Mytri, A.D. Rajkumar, D.N.Reddy and K. "Embedded Microcontroller based Digital Telemonitoring System for ECG", J. Instrum.Soc. India 37(2) 134-149.

[15]Dr. P. K. Dash, "Electrocardiogram Monitoring", Indian J. Anaesth. 2002; 46 (4): 251-256.